# QUICK GUIDE

**COMPASS GPS**

# SELECTION

## Introduction

This guide deals with the SELECTION theme in COMPASS GPS.

| | |
|---|---|
| ⚠ | Some hearing aids have a maximum sound pressure level exceeding 132 dB SPL. Take extra care when you work with these hearing aids, since they are able to give a harmful sound pressure level. COMPASS GPS shows a warning dialogue box when you select high-power hearing aids. |

When using REMOTE CARE please notice:


| | |
|---|---|
| ⚠ | REMOTE CARE is only intended for hearing aid users above the age of 18.<br>REMOTE CARE is not intended for hearing aid users who use a high-power hearing aid or high-power receiver for one or both ears. |

## Select hearing aid

In the middle of the window you can select specific series, models, etc. by means of drop-down lists and buttons. Use the buttons to see RIC/RITE, BTE, ITE and CIC hearing aids, and use the six drop-down lists to filter the hearing aids so you see only models with the desired elements.

If you select a button, for example the *CIC* button, all available CIC models are displayed at the bottom of the window. If you choose the *BTE* button as well, all available CIC and BTE models are displayed. The drop-down lists are the same – you can filter what you want to be displayed.


If you select the *Mark appropriate fitting range* check box, you can see a check mark beneath those hearing aids at the bottom of the window where your client's audiogram falls within the fitting range.

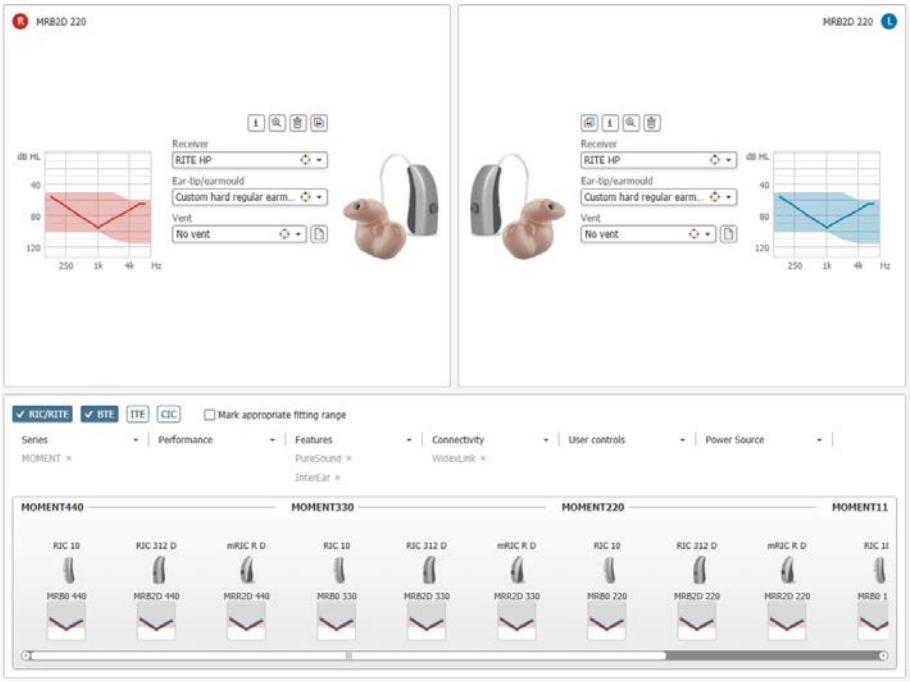


At the bottom of the window you can see all available hearing aids, depending on your choices in the middle of the window. You now have a customized view of the hearing aids, in the sense that you choose which hearing aids you want to see. Use the horizontal scroll bar to see all available hearing aids.

## Hearing aid information

Use your mouse-pointer to choose a set of hearing aids. When you hold the mouse pointer over a hearing aid, select either the red R icon for the right ear, the blue L icon for the left ear, or the red and blue icon in the middle for both ears. Once you have chosen a set of hearing aids, you can see them at the top of the workspace. Each of the panes contains the following information:

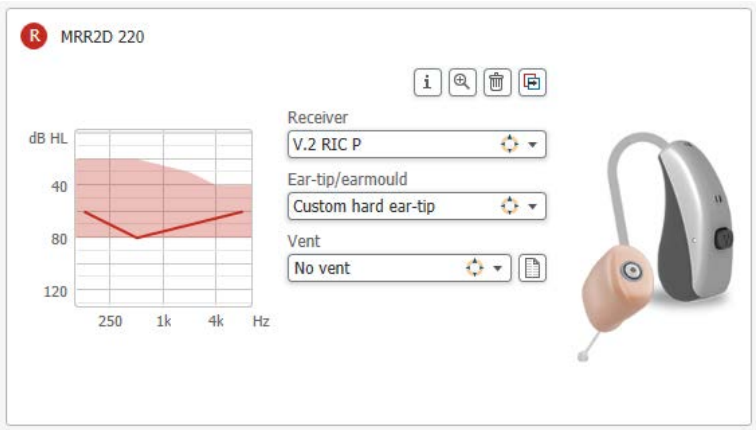


- Model name of the hearing aid, next to either a red R icon for the right hearing aid or a blue L icon for the left hearing aid
- Audiogram
- Fitting range
- Drop-down lists for the selection of EarWare (depending on the hearing aid model)
- Information button (information about the hearing aid)

- Zoom button
- Delete button
- Copy EarWare button
- Illustration of the hearing aid (when you select a piece of EarWare, the hearing aid illustration is shown with the EarWare)
- Button to open the Vent conversion table that can help you choose the correct vent for your client's ear-tip/earmold.

*For further information and guidance, open the Help system from the top navigation bar in the COMPASS GPS program, or by pressing the F1 button on your keyboard.*

This document is supplied in electronic form. A paper version of this instruction can be requested at no additional cost on http://widex.pro/gps-startup-guide, expected delivery time 7 calendar days. The document is also available on http://widex.pro/gps-startup-guide.

© Widex. All rights reserved

Document version: 2.0. Issued: 2019-11