QUICK GUIDE

COMPASS GPS

TRANSFER SETTINGS

Introduction

This quick guide explains the Transfer settings tool in COMPASS GPS. You can find the tool under the SESSION START theme. Transfer settings lets you copy hearing aid settings from one hearing aid to another.

Before you use the tool

The Transfer settings tool is not available for all hearing aid series. You can transfer settings between different performance levels, different models and with different EarWare, as long as the hearing aids are of the same series.

If the hearing aids used for receiving data have already been fitted to another client - and thus might contain data that does not suit your client - your client must NOT wear the hearing aids before the Transfer settings process is completed.

EVOKE/MOMENT – SoundSense Adapt
If you would like the transfer to include any SoundSense Adapt data that your client has generated while trying out the previous hearing aids at home, you must first export the data from the hearing aids to the database and save the export as a new session. Then select the new session as the base of your transfer when going through the Transfer settings flow.

Note that the Transfer settings feature imports settings, not sound.

Import data

To import data from a saved session:

1. Select *Transfer settings* in the SESSION START window. The *Import data* tab opens in the Transfer settings window.

2. Place the hearing aids close to the programming interface on your desk (it is NOT recommended to transfer the settings while the hearing aids are in your client's ears).

3. Click *Select database session* to get a list of all valid sessions to import from your database.


4. All valid sessions are shown, with the newest on top. Select the session you want to import, prepare the new hearing aids for connection, and select *Connect to new HA*.


5. Detected hearing aids are shown. Select the correct hearing aids, select side, and click *Next*.


6. COMPASS displays the connected hearing aids with the EarWare from the saved session. If it is possible to change the EarWare for the selected hearing aids, this option is accessible. Select the appropriate EarWare and acoustics. To confirm, click *Next*.


7. COMPASS displays an overview of imported data. This overview indicates which settings will be transferred, and how. All other settings will be set to default for the new hearing aids. This is the final step. If accepted, it is no longer possible to cancel the process. To accept, click *Import*.

8. COMPASS imports the data, and the process is completed.

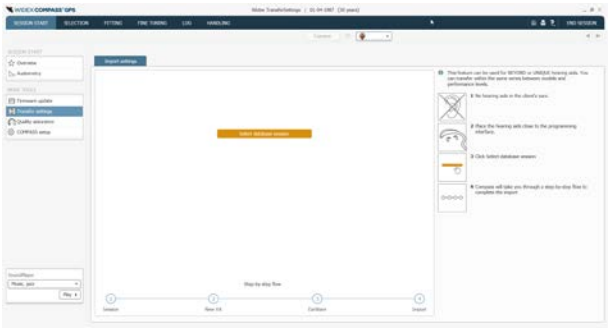

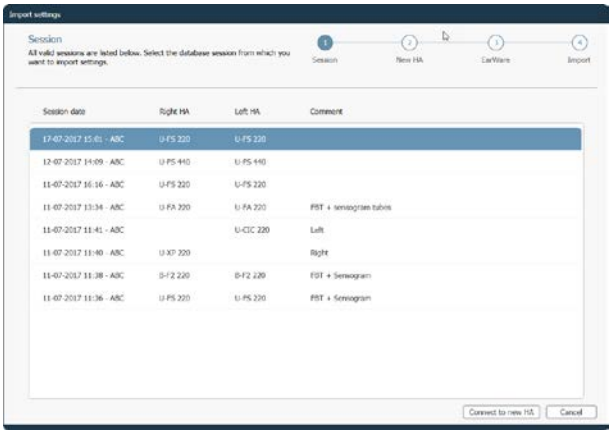

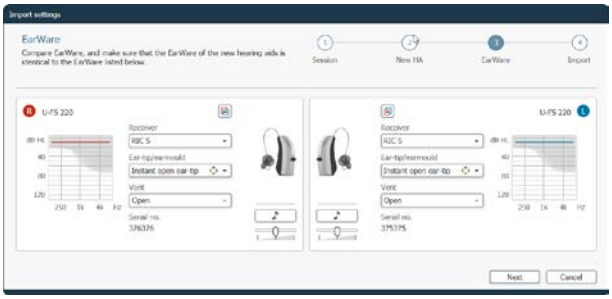

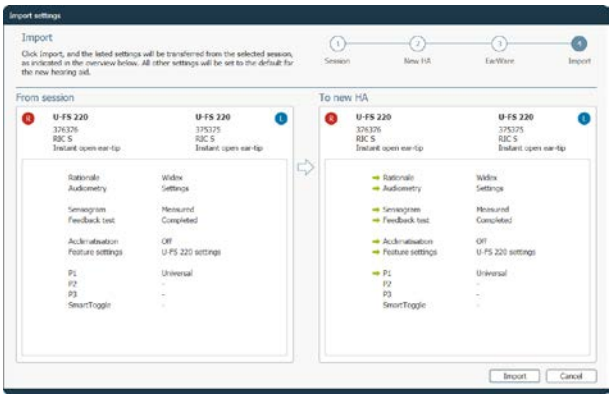

Details about the import

Note the following regarding the import

- All audiometric data is imported to the new hearing aids. Programs, sound classes and feature settings are imported, if possible.
- Adaptation settings are imported. Special conditions may apply when Automatic adaptation is activated.
- All measured feedback and Sensogram values are imported, **if possible.** If the acoustic identity has been changed (change of model, receiver, earmoulds, wire/tubes etc.), feedback and Sensogram values are not imported and will need to be re-measured.
- All other settings are set to their recommended values. Acoustic indicators, User controls, InterEar configuration, and Clinic options are set to default.
- Any existing data in the new hearing aids are overwritten.
- Note that matchings of DEX/CROS/BiCROS or apps are not transferred. All matchings and pairings need to be made again.

For further information and guidance, open the Help system from the top navigation bar in the COMPASS program, or by pressing the F1 button on your keyboard.

This document is supplied in electronic form. A paper version of this instruction can be requested at no additional cost on http://widex.pro/gps-startup-guide, expected delivery time 7 calendar days. The document is also available on http://widex.pro/gps-startup-guide.

Copyright © Widex. All rights reserved.

Document version: 2.0. Issue date: 2019-11